




SET UP IN THREE EASY STEPS

Step one:


Connect Mostcare Up

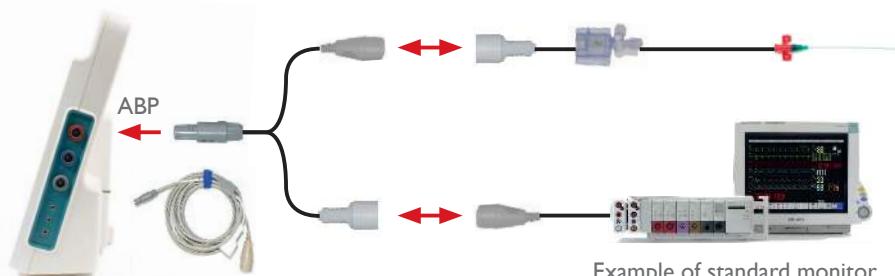

Connect the Y cable between the bedside monitor and the ABP transducer

or

Connect the analogue cable between Mostcare Up and the bedside monitor

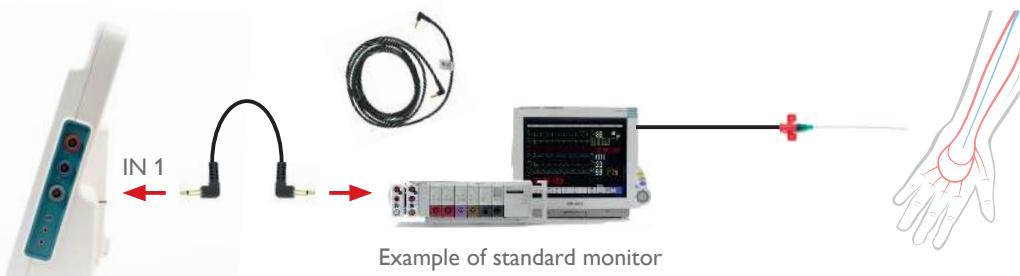

Scan with your smartphone

to view online or visit vygon.co.uk/mostcareeupevaluation/

Tel: 01793 748800 Copyright Vygon (UK) Ltd 2022 Content correct as of: 01/2022 Code: V00612 v5



Step two:

Enter patient data


1. Press **New monitoring**
2. Enter patient weight and height
3. Select ABP transducer and tick the **Y cable** box if applicable
4. Check other settings and press **Begin monitoring**



Step three:

Zero the transducer

- Place the transducer at the level of the phlebostatic axis
- Open the transducer stopcock to measure the atmospheric pressure
- Touch the curve on the screen and press **Zero ABP**
- Zero the primary monitor and re-establish trace

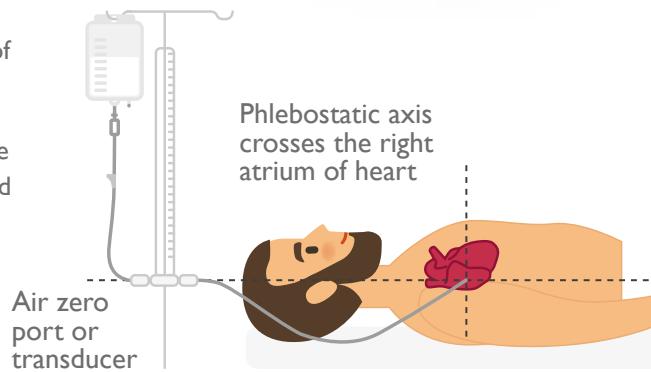

Scan with your smartphone

to view online or visit vygon.co.uk/mostcareeuevaluation/

